



How many tooth colors are there?

Sascha Hein^{a,*}, Ján Morovič^b, Peter Morovič^c, Omnia Saleh^{d,e}, Jörg Luchtenborg^e, Stephen Westland^a

^a School of Design, University of Leeds, Leeds, UK

^b HP Large Format Printing, HP Inc., Colchester, UK

^c HP Large Format Printing, HP Inc., Sant Cugat del Valles, Spain

^d Department for Restorative Science and Biomaterials Boston University, Boston, USA

^e Medical Center – University of Freiburg, Center for Dental Medicine, Department of Prosthetic Dentistry, Faculty of Medicine, University of Freiburg, Germany

ARTICLE INFO

Keywords:

Tooth color
Shade guides
Coverage error
Cardinality
CIELAB

ABSTRACT

Objectives: This study aimed to estimate the number of distinct tooth colors using a large dataset of in-vivo CIELAB measurements. It further assessed the coverage error (CE) and coverage error percentage (CEP) of commonly used shade guides and determined the number of shades needed for an ideal guide, using the Euclidean distance (ΔE_{ab}) and thresholds for clinical perceptibility (PT) and acceptability (AT) as evaluation criteria.

Methods: A total of 8153 untreated maxillary and mandibular anterior teeth were measured in vivo using calibrated dental photography. Cardinality was applied to determine the number of unique natural tooth colors. The CE and CEP were calculated for the Vita Classical and Vita 3D-Master shade guides, while the cardinality method was also used to estimate the number of shades required to adequately cover the estimated gamut of natural tooth colors.

Results: The cardinality analysis revealed 1173 unique natural tooth colors. The CE for the Vita Classical shade guide was 4.1 ΔE_{ab} , with a CEP of 75 % beyond AT, while the 3D-Master shade guide had a CE of 3.3 ΔE_{ab} and a CEP of 70 % beyond AT. Based on cardinality computation, 92 discrete shades are required to adequately cover the estimated gamut of natural tooth colors with a CE of 1.2 ΔE_{ab} and CEP of 0.3 % beyond AT.

Conclusions: Cardinality computations estimated 1173 unique tooth colors while 92 discrete shades are estimated for full coverage. Such a number is impractical for physical shade guides, but new digital tools and 3D printing may offer future solutions. Both, the Vita Classical and 3D-Master shade guides do not fully represent the range of natural tooth colors.

Clinical significance: This study highlights the limitations of existing shade guides and underscores the potential for new developments.

1. Introduction

Accurate shade matching, particularly for challenging single anterior restorations, remains a critical task in restorative dentistry. Clinicians frequently report complications with shade matching [1–3], which often leads to patient dissatisfaction [4] and a significant re-make rate [5]. Studies which have compared the benefits of instrumental shade measurement with visual shade selection [6–8] commonly agree that the latter is more subjective and less reliable [9,10], yet it remains the most common approach to shade matching in dentistry [11]. Vita Classical and Vita 3D-Master are the two most popular shade guides for visual

shade selection [12].

Despite their widespread use, the coverage error (CE) or its percentage (CEP) associated with these shade guides (i.e., the average distance between a natural tooth color and the closest shade tab [13]) often exceeds the threshold for clinical acceptability [13–22]. Studies have analyzed sample populations ranging from 60 [18] to 2067 [19] human teeth with reported CEs between 2.5 [22] and 8.4 [20] ΔE_{ab} units. This significant error has led to the development of hypothetical shade guides designed either to reduce the CE with the same number of shade tabs [16] or to maintain the same error with fewer tabs [14,23], thereby simplifying the shade matching process. However, none of these

* Correspondence to: Graduate School of Color Science and Technology, School of Design, University of Leeds, Woodhouse Lane, Leeds LS2 9JT, UK.

E-mail address: sdsch@leeds.ac.uk (S. Hein).

<https://doi.org/10.1016/j.dental.2024.10.016>

Received 29 September 2024; Received in revised form 25 October 2024; Accepted 25 October 2024

Available online 29 October 2024

0109-5641/© 2024 The Author(s). Published by Elsevier Inc. on behalf of The Academy of Dental Materials. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>).

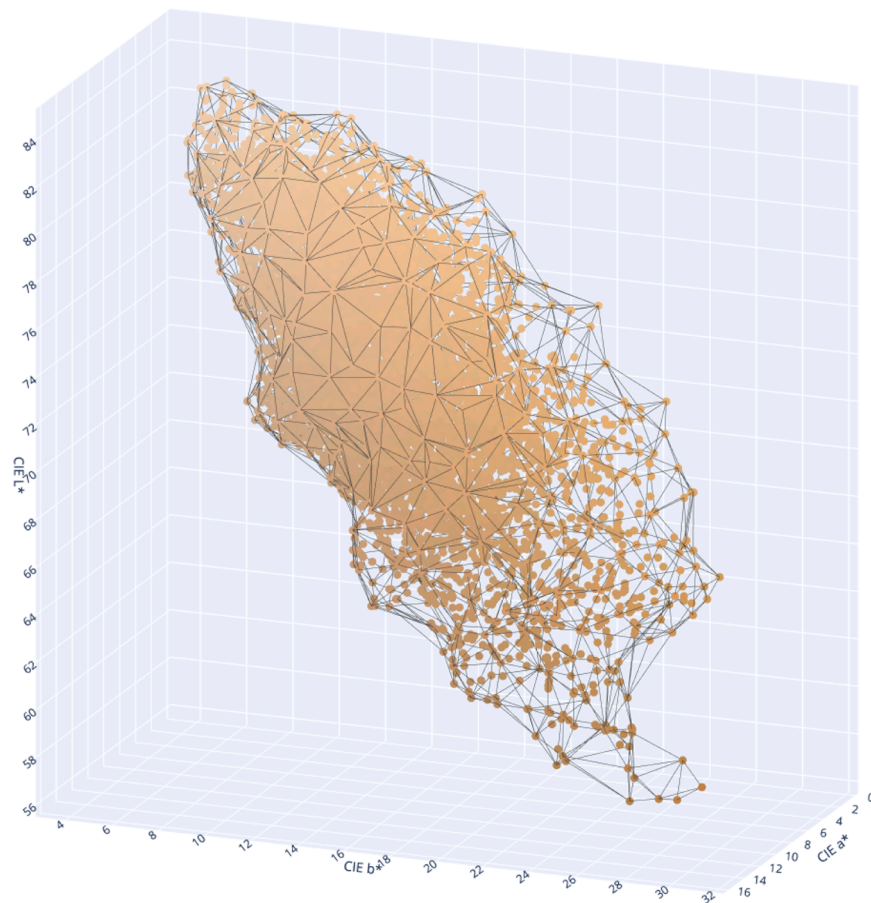


Fig. 1. Alpha hull representation of volume enclosing 8153 natural tooth colors measured in vivo in CIELAB color space ($\alpha = 2 \Delta E_{ab}$).

suggested improvements have found their way into new shade guides to enhance clinical practice. Determining the optimal number of samples for an ideal shade guide requires consideration of several factors, including the chosen visual acceptance threshold and the gamut of natural tooth colors, which remains elusive.

Cardinality is a mathematical concept that counts the number of distinct elements in a set [24]. Understanding the cardinality of natural tooth colors—how many unique, visually distinguishable tooth colors exist—based on measured CIELAB data from a representatively large population allows for the estimation of the number of shades needed for an ideal shade guide, improving representation and shade matching accuracy in dentistry.

The eLAB system is a color measurement tool that utilizes calibrated RAW images captured with a DSLR or mirrorless camera equipped with a macro lens and a ring or lateral flash [25]. Cross-polarization is used to eliminate specular reflections from the tooth surface [26] to allow for unobstructed color measurement [27–29] regardless of ambient light conditions [30]. For consistent tooth color representation across different digital cameras, a gray reference card is used, equipped with a color checker consisting of 22 patches [31] which serve for computing a transformation matrix that relates their sRGB values to known CIELAB values. This matrix is then applied to the entire image, converting sRGB to CIELAB and subsequently back to sRGB for accurate color rendering based on the reference CIELAB data [32]. This process ensures standardization across images from different cameras, allowing for direct comparison of tooth colors [33]. The eLAB system has been used to detect tooth color changes comparable to spectrophotometric analysis [34] and to monitor changes in white spot lesions (WSLs) as a function of treatment [35]. It has been used to analyze the shade variance of identically labeled direct composite materials from different

manufacturers [36] and to assess the efficiency of at-home bleaching protocols [37]. A recent multicenter study demonstrated that the eLAB system achieved visual-instrumental agreement with no significant difference in performance compared to other commonly mentioned color measurement devices including spectrophotometer, multispectral cameras and tele-spectroradiometers [38].

The aims of this study were to first estimate the number of distinct tooth colors using a large dataset of in-vivo CIELAB measurements obtained from the eLAB system, then to identify a set of hypothetical ‘super shades’ to best cover the gamut of natural tooth colors, and finally to assess the CE, CEP, and the frequency of individual shades for both, the most common shade guides and the identified super shades.

2. Material and methods

2.1. Study design

This study was conducted following the approval of the research ethics committee, granted under reference number 1366. All procedures adhered to ethical guidelines and received necessary consent from participants, in compliance with the EU’s General Data Protection Regulation (GDPR).

2.2. Data collection

Over 29 months, a total of 121,198 RAW images were collected from users of the eLAB_prime shade matching software (Emulation, Freiburg, Germany) across 98 countries worldwide. A multi-step AI-based approach was utilized to vet the data pool. A convolutional neural network was used to assess and filter images based on quality metrics

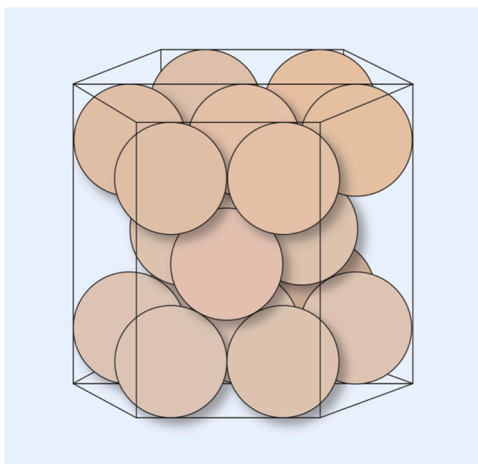


Fig. 2. Example of hexagonal close-packed sphere model of visually distinguishable tooth colors used in this study. The diameter of each sphere corresponds to the clinical threshold chosen.

[39,40], such as correct exposure, presence of a grey reference card. For duplicate detection, feature extraction followed by clustering and perceptual hashing was used [41,42]. Object detection and semantic segmentation models [43] identified and excluded images with artificial

restorations. The resulting pool of images was further examined visually by five experienced master dental technicians using the eLAB_prime software (Emulation, Freiburg, Germany). This resulted in a total of 2038 RAW images to be included for the CIELAB tooth color measurement of 8153 untreated maxillary and mandibular anterior incisors.

Color measurements were taken across the incisal and medio-cervical regions of the labial surface, providing a broad representation of the tooth's color. The final color was calculated as the average of these CIELAB values, consistent with methodologies used in other studies [37, 44–46].

For each Vita Classical (VC) and 3D Master (3D) shade tab, their colorimetric data were obtained using the eLAB system, following the same method used for the natural tooth color population. The reference numbers for the shade guides were +J017B0271 for VC and +J017B36002 for 3D.

2.3. Computation of cardinalities

The required condition to answer the question of how many tooth colors exist is that each color is unique, with no other color matching it. In a finite, countable set of numbers—such as tooth colors, which occupy only a small region of the CIELAB color space—cardinality simply refers to the number of unique elements in that set. Therefore, working with a restricted set of elements makes this task manageable, unlike trying to determine how many colors there are in total, from a set of infinite or practically infinite elements [47,48].

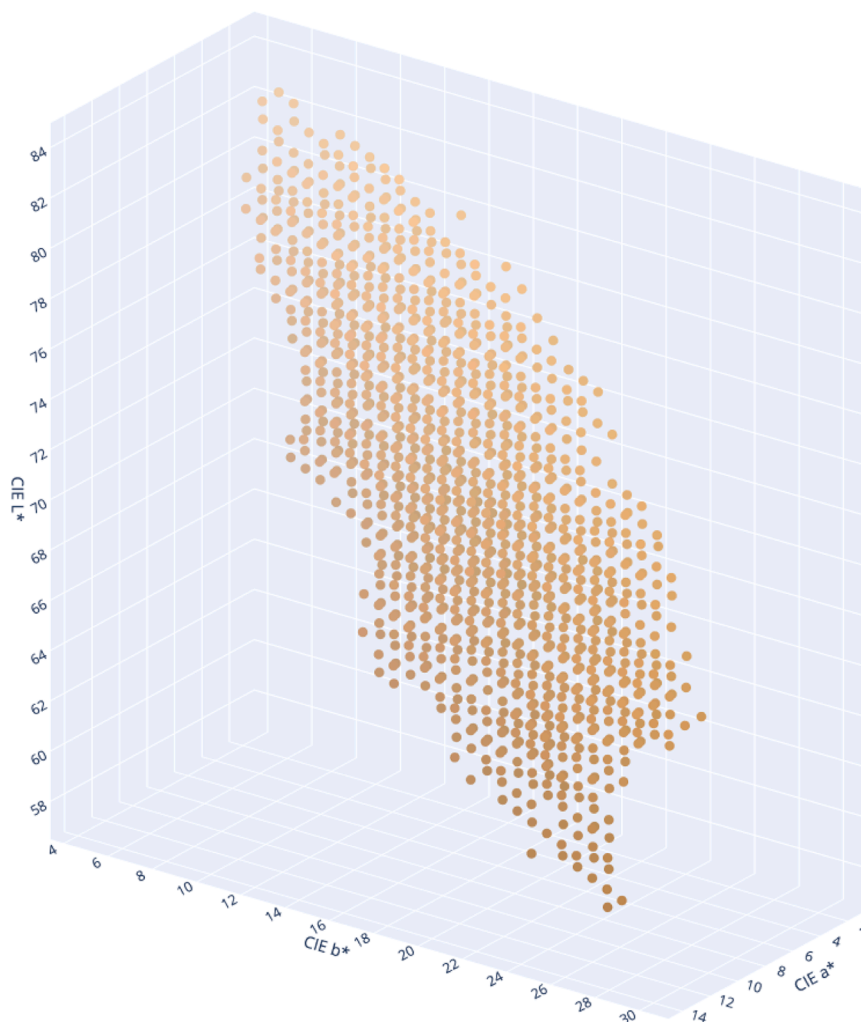


Fig. 3. Depiction of cardinalities revealing 1173 unique natural tooth colors.

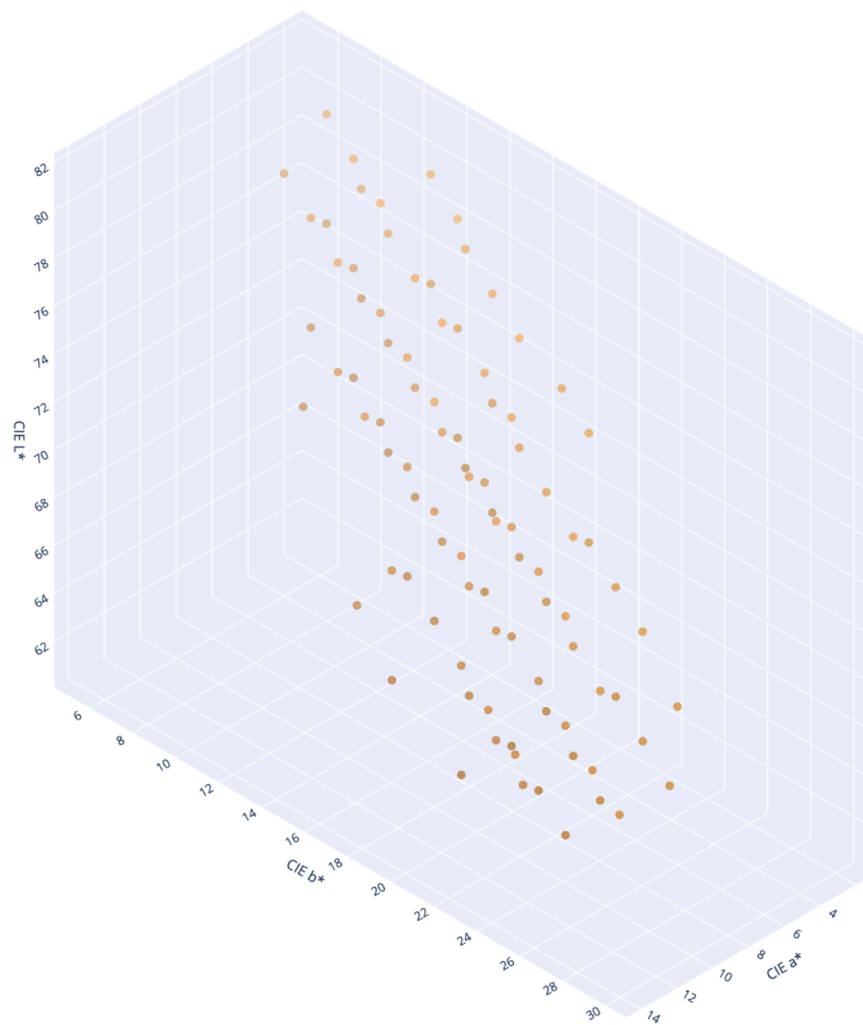


Fig. 4. Representation of 92 super shades, indicating minimum number of shade tabs required for an ideal shade guide.

First, an appropriate color difference metric needed to be nominated. In this case the CIE 1976 ΔE_{ab} formula was chosen because a recent multicenter study [38] demonstrated that the eLAB system achieved an outstanding 82 % visual-instrumental agreement using ΔE_{ab} , outperforming much more complex color difference equations such as CIEDE2000 and CAM16-UCS.

Next, a volume space containing 8153 natural tooth coordinates S in CIELAB color space was used for the efficient construction of a convex hull called an α -shape which presents the hull containing all points of S such that no more than three hull vertices are contained in a sphere of radius α [49]. In this context, α is a sufficiently small, positive real number chosen to construct a boundary of the natural tooth color gamut such that its value represents a desired level of tolerance to concavity. In the present case a value of $\alpha = 2 \Delta E_{ab}$ units was chosen for the construction of the convex hull since it provided a good balance between the density of S and the low thresholds used for perceptibility and acceptability in dentistry [50] (Fig. 1). Then, a custom Python routine (Python Software Foundation, Wilmington, DE, USA) was employed to quantify the cardinality of the most densely packed set of unique colors in the α -shape of natural tooth shades, ensuring that the difference between any two points is greater than or equal to the threshold for clinical perceptibility, set at $1.2 \Delta E_{ab}$ units [50]. This was achieved with a hexagonal closed sphere-packing model [51], where each tooth color was represented by a sphere with its center at that color and with a diameter matching the corresponding ΔE_{ab} threshold value of $1.2 \Delta E_{ab}$. The number of non-overlapping spheres within the dataset indicated the

cardinality, providing a measure of distinct tooth colors (Fig. 2).

2.4. Identifying super shades

To identify a set of ‘super shades,’ representing hypothetical tooth colors that best cover the range of natural tooth colors, the cardinality calculation was repeated. The goal of an ideal shade guide is to provide adequate coverage of the natural tooth color gamut within the clinically acceptable range, while remaining as practical as possible. Therefore, the same convex hull and sphere packing model was employed, but with the sphere diameter was set to $2.7 \Delta E_{ab}$ units corresponding to the threshold for clinical acceptability [50].

2.5. Computation of coverage error and coverage error percentage

To compute the CE and the CEP for the VC and 3D shade guides, the color differences between each of the 8153 sample tooth colors and each reference shade tab from both shade guides were calculated under Illuminant D65 and for the CIE 1931 standard colorimetric observer [52] using the ΔE_{ab} color difference equation in MATLAB (MathWorks, Natick, MA, USA). For each natural tooth color, the reference shade tab with the minimum color difference was identified, and the frequency of each reference shade tab being the closest match was recorded. The CE was determined by averaging the minimum ΔE_{ab} values across all sample tooth colors using this formula:

Table 1
CE and CEP along with standard deviations (SD) for the Vita Classical (VC) and for the 3D-Master (3D) shade guides respectively.

Shade Guide	CE (ΔE_{ab}) (SD)	CEP \leq PT (SD)	CEP $>$ PT, \leq AT (SD)	CEP $>$ AT (SD)
VC	4.1 (1.8)	1.1 % (0.2)	24.3 % (0.4)	74.6 % (1.6)
3D	3.3 (1.4)	3.0 % (0.2)	27.8 % (0.7)	70.3 % (1.2)
Super Shades	1.2 (0.4)	33.8 % (0.2)	65.9 % (0.3)	0.3 % (1.5)

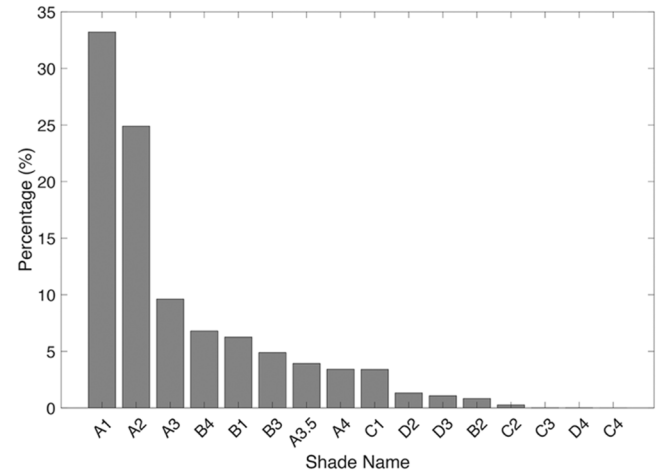


Fig. 5. Percentages of shade frequency for Vita Classical shades.

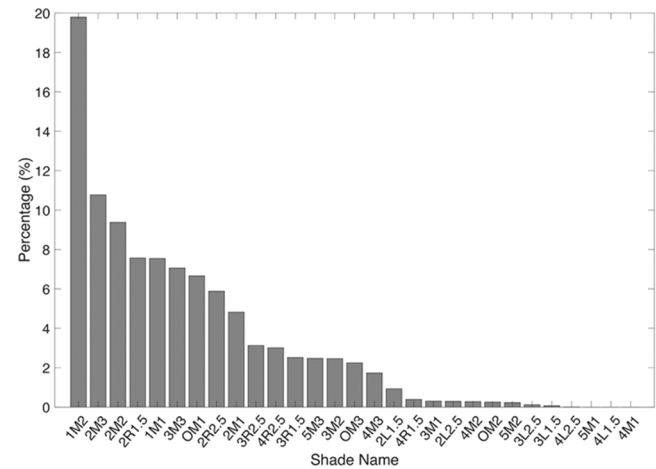


Fig. 6. Percentages of shade frequency for Vita 3D-Master shades.

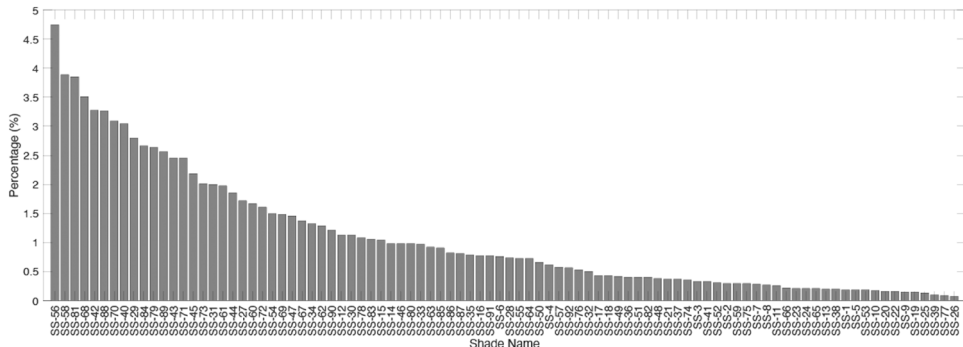


Fig. 7. Percentages of shade frequency for 92 super shades (SS).

$$CE = \frac{\sum_{i=1}^n \min(\Delta E_i)}{n}$$

To express the CEP, the proportion of occurrences for each shade tab was calculated and normalized by the total number of sample tooth colors using this formula:

$$CEP_j = \left(\frac{\text{occurrences}_j}{n} \right) \times 100$$

The resulting percentages were then sorted from high to low, to facilitate a comparative analysis. Accordingly, the same computations were carried out to evaluate the effectiveness of super shades.

3. Results

3.1. Cardinalities and super shades

Based on the threshold for clinical perceptibility (ΔE_{ab} 1.2), the computation of cardinalities revealed 1173 unique natural tooth colors (Fig. 3) and 92 super shades when the thresholds for clinical acceptability (ΔE_{ab} 2.7) was used, representing the minimum number of shade tabs that an ideal shade guide would need (Fig. 4).

3.2. Coverage error of shade guides and super shades

Table 1 lists the CE and CEP results for VC, 3D shade guides and the super shades, along with their standard deviations. Fig. 5 shows the percentages for the most common shades of the VC shade guide while Fig. 6 displays the corresponding values for the 3D shade guide and Fig. 7 for the super shades.

4. Discussion

This study aimed to estimate the number of distinct tooth colors based on 8153 in-vivo CIELAB measurements and to determine the CE and CEP of the most common shade guides alongside a set of hypothetical ‘super shades’.

Previous studies have reported similar CEs for the VC and 3D shade guides, averaging 4.4 ΔE_{ab} and 4.2 ΔE_{ab} , respectively [13–22,53–57]. Our findings align with these reports, confirming that while widely used, current shade guides are limited in covering the full range of natural tooth colors. Using cardinality computation, this study estimated that a set of 92 super shades could potentially cover the gamut of natural tooth colors with a CEP of only 0.3 % outside the threshold for clinical acceptability.

The reported frequencies of individual shades with the lowest CEP also vary considerably. The findings of this study are generally in agreement with those of Ruiz Lopez et al. [22] and Paravina et al. [16] but differ from Bayindir et al. [15] and Tabatabaian et al. [21], who both reported that the VC shade ‘D3’ had the lowest CEP frequency.

While training programs for visual shade matching have been

proposed [58–61] the present study highlights the persistent challenges in achieving accurate shade matches, even with training. Recent research has also focused on evaluating the accuracy of shade measurement devices [7,9,62–64] and, more recently, intraoral scanners [7, 65,66]. However, the results of this study suggest that discrepancies in shade matching may stem more from the coverage error of shade guides than from device accuracy [67].

Although a physical shade guide consisting of 92 discrete shades would be highly impractical, the insights from the present study could prove beneficial in the near future with the rise of digital tools for shade matching [31,68] and new technology like 3D printing [69].

Tooth color appearance is a complex phenomenon [70] and cannot be fully captured by CIELAB values alone. In clinical practice, acceptance or rejection of a restoration often depends on situational factors that cannot be wholly accounted for by visual thresholds alone. For instance, a clinical study by Ballard et al. [57] found that 94 % of patients were at least satisfied or extremely satisfied with a clinical shade-match that was well beyond the clinical acceptability threshold assumed in the present study.

It is also important to recognize that the results of the cardinality computation depend on specific input parameters, such as the definition of alpha-radii and the chosen visual threshold values. Consequently, the results are accurate for color differences computed using Euclidean distance but may not hold for other color difference equations. This is because the volume of the alpha hull, and how many spheres can be packed within it, is determined by the visual thresholds and the color difference equation used, which in turn define the diameter of each sphere. However, even with variations in these parameters, the overall finding remains consistent: a significantly larger number of shade tabs is needed for an ideal shade guide than is currently available.

5. Conclusion

To the best of our knowledge, the present study comprises the largest gamut of natural tooth colors ever published. Unfortunately, the results show that the likelihood of selecting a shade that is either clinically imperceptible or at least acceptable is one in four for the VC shade guide (25 %) and nearly one in three for the 3D-Master shade guide (31 %). On the other hand, a physical shade guide to achieve almost complete coverage is estimated to require 92 discrete shade tabs. These findings highlight the inherent challenges when trying to select the right shade during daily clinical practice.

References

- [1] Lawson NC, Frazier K, Bedran-Russo AK, Khajotia S, Park J, Urquhart O. Zirconia restorations: an American Dental Association Clinical Evaluators Panel survey. *J Am Dent Assoc* (1939) 2021;152. <https://doi.org/10.1016/j.adaj.2020.10.012>. 80-1.e2.
- [2] Alnusayri MO, Sghaireen MG, Mathew M, Alzarea B, Bandela V. Shade selection in esthetic dentistry: a review. *Cureus* 2022;14:e23331. <https://doi.org/10.7759/cureus.23331>.
- [3] Paravina R, Stanković D, Aleksov L, Mladenović D, Ristić K. Problems in standard shade matching and reproduction procedure in dentistry: a review of the state of the art. *Facta Univ, Serb* 1997;4:12–6.
- [4] Kawaragi C, Ishikawa S, Miyoshi F, Furukawa K, Ishibashi K. Evaluations by dentists and patients concerning the color of porcelain-fused-to-metal restoration. *Dent J Iwate Med Univ* 1990;15:9–17. <https://doi.org/10.20663/iwateshigakukaishi.15.1.9>.
- [5] Corcodel N, Zenthöfer A, Setz J, Rammelsberg P, Hassel AJ. Estimating costs for shade matching and shade corrections of fixed partial dentures for dental technicians in Germany: A pilot investigation. *Acta Odontol Scand* 2011;69: 319–20. <https://doi.org/10.3109/00016357.2011.568964>.
- [6] Alnusayri MO, Sghaireen MG, Mathew M, Alzarea B, Bandela V. Shade selection in esthetic dentistry: a review. *Cureus* (Palo Alto, CA) 2022;14. <https://doi.org/10.7759/cureus.23331>. e23331-e.
- [7] Morsy N, Holiel AA. Color difference for shade determination with visual and instrumental methods: a systematic review and meta-analysis. *Syst Rev* 2023;12: 95. <https://doi.org/10.1186/s13643-023-02263-9>.
- [8] Chen H, Huang J, Dong X, Qian J, He J, Qu X, et al. A systematic review of visual and instrumental measurements for tooth shade matching. *Quintessence Int* 2012; 43:649–59.
- [9] Tabatabaian F, Beyabanaki E, Alirezaei P, Epakchi S. Visual and digital tooth shade selection methods, related effective factors and conditions, and their accuracy and precision: a literature review. *J Esthet Restor Dent* 2021;33:1084–104. <https://doi.org/10.1111/jerd.12816>.
- [10] Hardan L, Bourgi R, Cuevas-Suárez CE, Lukomska-Szymanska M, Monjarás-Ávila AJ, Zarow M, et al. Novel trends in dental color match using different shade selection methods: a systematic review and meta-analysis. *Materials* 2022;15:468. <https://doi.org/10.3390/ma15020468>.
- [11] Haddad HJ, Jakstat HA, Arnetzl G, Borbely J, Vichi A, Dumfahrt H, et al. Does gender and experience influence shade matching quality? *J Dent* 2009;37:e40–4. <https://doi.org/10.1016/j.jdent.2009.05.012>.
- [12] Paravina RD. Performance assessment of dental shade guides. *J Dent* 2009;37: e15–20. <https://doi.org/10.1016/j.jdent.2009.02.005>.
- [13] O'Brien WJ, Boenke KM, Groh CL. Coverage errors of two shade guides. *Int J Prosthodont* 1991;4:45–50.
- [14] Analoui M, Papkosta E, Cochran M, Matis B. Designing visually optimal shade guides. *J Prosthet Dent* 2004;92:371–6. <https://doi.org/10.1016/j.prosdent.2004.06.028>.
- [15] Bayindir F, Kuo S, Johnston W, Wee A. Coverage error of three conceptually different shade guide systems to vital unrestored dentition. *J Prosthet Dent* 2007; 98:175–85. [https://doi.org/10.1016/S0022-3913\(07\)60053-5](https://doi.org/10.1016/S0022-3913(07)60053-5).
- [16] Paravina RD, Majkic G, Imai FH, Powers JM. Optimization of tooth color and shade guide design. *J Prosthodont* 2007;16:269–76. <https://doi.org/10.1111/j.1532-849X.2007.00189.x>.
- [17] Yuan J, Brewer J, Monaco E, Davis E. Defining a natural tooth color space based on a 3-dimensional shade system. *J Prosthet Dent* 2007;98:110–9. [https://doi.org/10.1016/S0022-3913\(07\)60044-4](https://doi.org/10.1016/S0022-3913(07)60044-4).
- [18] Li Q, Yu H, Wang Y. In vivo spectroradiometric evaluation of colour matching errors among five shade guides. *J Oral Rehabil* 2009;36:65–70. <https://doi.org/10.1111/j.1365-2842.2008.01894.x>.
- [19] Haddad H, Salameh Z, Sadig W, Aboushelib M, Jakstat H. Allocation of color space for different age groups using three-dimensional shade guide systems. *Eur J Esthet Dent* 2011;6:94–102.
- [20] Rao D, Joshi S. Evaluation of natural tooth color space of the Indian population and its comparison to manufacturer's shade systems. *Contemp Clin Dent* 2018;9:395–9. <https://doi.org/10.4103/ccd.ccd.144.18>.
- [21] Tabatabaian F, Khezri A, Ourang S, Namdari M. Assessment of coverage error for two common commercial dental shade guides using a spectrophotometric method. *Color Res Appl* 2022;47:528–36. <https://doi.org/10.1002/col.22725>.
- [22] Ruiz-López J, Perez M, Lucena C, Pulgar R, López-Torruño A, Tejada-Casado M, et al. Visual and instrumental coverage error of two dental shade guides: an in vivo study. *Clin Oral Investig* 2022;26:5961–8. <https://doi.org/10.1007/s00784-022-04556-0>.
- [23] Cocking C, Helling S, Oswald M, Rammelsberg P, Reinelt G, Hassel AJ. Using discrete optimization for designing dental shade guides. *Color Res Appl* 2010;35: 233–9. <https://doi.org/10.1002/col.20547>.
- [24] Cantor G. Ueber unendliche, lineare Punktmannichfaltigkeiten. *Math Ann* 1879;15: 1–7. <https://doi.org/10.1007/BF01444101>.
- [25] Hein S, Zangl M. The use of a standardized gray reference card in dental photography to correct the effects of five commonly used diffusers on the color of 40 extracted human teeth. *Int J Esthet Dent* 2016;11:246–59.
- [26] Wander PA, Gordon PD. Dental photography. London: British Dental Association; 1987.
- [27] Mahn E, Tortora SC, Olate B, Cacciuttolo F, Kernitsky J, Jorquera G. Comparison of visual analog shade matching, a digital visual method with a cross-polarized light filter, and a spectrophotometer for dental color matching. *J Prosthet Dent* 2021; 125:511–6. <https://doi.org/10.1016/j.prosdent.2020.02.002>.
- [28] He WH, Park CJ, Byun S, Tan D, Lin CY, Chee W. Evaluating the relationship between tooth color and enamel thickness, using twin flash photography, cross-polarization photography, and spectrophotometer. *J Esthet Restor Dent* 2020;32: 91–101. <https://doi.org/10.1111/jerd.12553>.
- [29] Yilmaz B, Dede D, Diker E, Fonseca M, Johnston WM, Küçükenci AS. Effect of cross-polarization filters on the trueness of colors obtained with a single-lens reflex camera, macro lens, and a ring flash. *J Esthet Restor Dent* 2023;35:878–85. <https://doi.org/10.1111/jerd.13053>.
- [30] Farah RI, Almershed AS, Albahli BF, Al-Haj Ali SN. Effect of ambient lighting conditions on tooth color quantification in cross-polarized dental photography: a clinical study. *J Prosthet Dent* 2022;128:776–83. <https://doi.org/10.1016/j.prosdent.2021.01.015>.
- [31] Hein S, Modrić D, Westland S, Tomeček M. Objective shade matching, communication, and reproduction by combining dental photography and numeric shade quantification. *J Esthet Restor Dent* 2021;33:107–17. <https://doi.org/10.1111/jerd.12641>.
- [32] Westland S, Ripamonti C., Cheung V. Characterisation of Cameras. *Computational Colour Science using MATLAB* 2012. p. 143–157. <http://doi.org/10.1002/9780470710890.ch10>.
- [33] Hein S, Tapia J, Bazos P. eLABor aid: a new approach to digital shade management. *Int J Esthet Dent* 2017;12:186–202.
- [34] Bezerra AP, Oshima S, Feldmann A, Tango RN, Duque TM, Philippi AG, et al. Digital photocolormetric analysis of in vitro tooth color changes. *Oper Dent* 2024; 49:336–44. <https://doi.org/10.2341/23-134-1>.
- [35] Kashash Y, Hein S, Göstemeier G, Aslanalp P, Weyland MI, Bartzela T. Resin infiltration versus fluoride varnish for visual improvement of white spot lesions during multibracket treatment. A randomized-controlled clinical trial. *Clin Oral Investig* 2024;28:308. <https://doi.org/10.1007/s00784-024-05695-2>.

- [36] Notarantonio A, Seay A. A system for reliable composite shade matching: custom shade tabs and an intra-oral mockup. *J Esthet Restor Dent* 2023;35:787–95. <https://doi.org/10.1111/jerd.13106>.
- [37] Salehi A, He M, Hampé-Kautz V, Etienne O. Digital evaluation of dental bleaching using a new methodology: an in vivo study. *Int J Esthet Dent* 2022;17:448–67.
- [38] Hein S, Saleh O, Li C, Nold J, Westland S. Bridging instrumental and visual perception with improved color difference equations: a multi-center study. *Dent Mater* 2024. <https://doi.org/10.1016/j.dental.2024.07.003>.
- [39] Li Z, Liu F, Yang W, Peng S, Zhou J. A survey of convolutional neural networks: analysis, applications, and prospects. *IEEE Trans Neural Netw Learn Syst* 2022;33: 6999–7019. <https://doi.org/10.1109/TNNLS.2021.3084827>.
- [40] Jeong HK, Park C, Jiang SW, Nicholas M, Chen S, Henao R, et al. Image Quality Assessment Using Convolutional Neural Network in Clinical Skin Images. *JID Innov* 2024;4:100285. <https://doi.org/10.1016/j.xjidi.2024.100285>.
- [41] Vishal M, Banerjee A, Evans BL. A clustering based approach to perceptual image hashing. *IEEE Trans Inf Forensics Secur* 2006;1:68–79. <https://doi.org/10.1109/TIFS.2005.863502>.
- [42] Xudong L, Wang ZJ. Perceptual Image hashing based on shape contexts and local feature points. *IEEE Trans Inf Forensics Secur* 2012;7:1081–93. <https://doi.org/10.1109/TIFS.2012.2190594>.
- [43] Dong J, Chen Q, Yan S, Yuille A. Towards Unified Object Detection and Semantic Segmentation. Cham: Springer International Publishing. p. 299–314. http://doi.org/10.1007/978-3-319-10602-1_20.
- [44] Dias S, Dias J, Pereira R, Silveira J, Mata A, Marques D. Different methods for assessing tooth colour-in vitro study. *Biomim (Basel)* 2023;8. <https://doi.org/10.3390/biomimetics8050384>.
- [45] Ishizaki T. Chromatic research on the spectral radiance factors of teeth: maxillary anterior teeth. *Nihon Hotetsu Shika Gakkai Zasshi* 1989;33:771–85. <https://doi.org/10.2186/jjps.33.771>.
- [46] Tabatabaia F, Khezri AS, Ourang SA, Namdari M. Assessment of coverage error for two common commercial dental shade guides using a spectrophotometric method. *Color Res Appl* 2022;47:528–36. <https://doi.org/10.1002/col.22725>.
- [47] Morovic J, Cheung V, Morovic P. Why we don't know how many colors there are. *Proc IS&T CGIV 2012 6th European Conf on Colour in Graphics, Imaging, and Vision* 2012. p. 49–53. <http://doi.org/10.2352/CGIV.2012.6.1.art00009>.
- [48] Kuehni RG. How many object colors can we distinguish? *Color Res Appl* 2016;41: 439–44. <https://doi.org/10.1002/col.21980>.
- [49] Edelsbrunner H, Mücke EP. Three-dimensional alpha shapes. *ACM Trans Graph* 1994;13:43–72. <https://doi.org/10.1145/174462.156635>.
- [50] Paravina RD, Ghinea R, Herrera LJ, Bona AD, Igiel C, Linninger M, et al. Color difference thresholds in dentistry. *J Esthet Restor Dent* 2015;27:S1–9. <https://doi.org/10.1111/jerd.12149>.
- [51] Morovic P, Morovic J. On the cardinality of color stimulus properties. *Color Imaging Conf* 2023:178–86. <https://doi.org/10.2352/CIC.2023.31.1.34>.
- [52] PD ISO/TR 28642:2016: Dentistry. Guidance on colour measurement. British Standards Institute; 2016.
- [53] Cocking C, Cevirgen E, Helling S, Oswald M, Corcoral N, Rammelsberg P, et al. Colour compatibility between teeth and dental shade guides in Quinquagenarians and Septuagenarians. *J Oral Rehabil* 2009;36:848–55. <https://doi.org/10.1111/j.1365-2842.2009.02003.x>.
- [54] Hassel A, Nitschke I, Rammelsberg P. Comparing lab color coordinates for natural teeth shades and corresponding shade tabs using a spectrophotometer. *Int J Prosthodont* 2009;22:72–4.
- [55] Wang P, Wei J, Li Q, Wang Y. Evaluation of an optimized shade guide made from porcelain powder mixtures. *J Prosthet Dent* 2014;112:1553–8. <https://doi.org/10.1016/j.prosdent.2014.06.007>.
- [56] Dozic A, Voit N, Zwartser R, Khashayar G, Aartman I. Color coverage of a newly developed system for color determination and reproduction in dentistry. *J Dent* 2010;38:e50–6. <https://doi.org/10.1016/j.jdent.2010.07.004>.
- [57] Ballard E, Metz MJ, Harris BT, Metz CJ, Chou J-C, Morton D, et al. Satisfaction of dental students, faculty, and patients with tooth shade-matching using a spectrophotometer. *J Dent Educ* 2017;81:545–53. <https://doi.org/10.21815/JDE.016.022>.
- [58] Ristic I, Stankovic S, Paravina RD. Influence of color education and training on shade matching skills. *J Esthet Restor Dent* 2016;28:287–94. <https://doi.org/10.1111/jerd.12209>.
- [59] Samra APB, Moro MG, Mazur RF, Vieira S, De Souza EM, Freire A, et al. Performance of dental students in shade matching: impact of training. *J Esthet Restor Dent* 2017;29:E24–32. <https://doi.org/10.1111/jerd.12287>.
- [60] Alfouzan AF, Alqahtani HM, Tashkandi EA. The effect of color training of dental students' on dental shades matching quality. *J Esthet Restor Dent* 2017;29:346–51. <https://doi.org/10.1111/jerd.12284>.
- [61] Capa N, Malkondu O, Kazazoglu E, Calikkocaoglu S. Effects of individual factors and the training process of the shade-matching ability of dental students. *J Dent Sci* 2011;6:147–52. <https://doi.org/10.1016/j.jds.2011.04.001>.
- [62] Rashid F, Farook TH, Dudley J. Digital shade matching in dentistry: a systematic review. *Dent J* 2023;11:250. <https://doi.org/10.3390/dj11110250>.
- [63] Dudkiewicz K, Łacinek S, Jedliński M, Janiszewska-Olszowska J, Grocholewicz K. A clinician's perspective on the accuracy of the shade determination of dental ceramics—a systematic review. *J Pers Med* 2024;14:252. <https://doi.org/10.3390/jpm14030252>.
- [64] Crespo PC, Córdova AK, Palacios A, Astudillo D, Delgado B. Variability in tooth color selection by different spectrophotometers: a systematic review. *Open Dent J* 2022;16. <https://doi.org/10.2174/18742106-v16-e221124-2022-48>.
- [65] Tabatabaia F, Namdari M, Mahshid M, Vora SR, Mirabbasi S. Accuracy and precision of intraoral scanners for shade matching: a systematic review. *J Prosthet Dent* 2022. <https://doi.org/10.1016/j.prosdent.2022.08.034>.
- [66] Mehl AC, Bosch G, Fischer CAI, Ender A. In vivo tooth-color measurement with a new 3D intraoral scanning system in comparison to conventional digital and visual color determination methods. *Int J Comput Dent* 2017;20(4):343–61.
- [67] Kim HK. Evaluation of the repeatability and matching accuracy between two identical intraoral spectrophotometers: An in vivo and in vitro study. *J Adv Prosthodont* 2018;10:252–8. <https://doi.org/10.4047/jap.2018.10.3.252>.
- [68] Awdaljan M, Roque J, Choi J, Rondon L. Introducing a novel approach to dental color reproduction using AI technology. *J Esthet Restor Dent* 2024. <https://doi.org/10.1111/jerd.13300>.
- [69] Espinar C, Della Bona A, Pérez MM, Pulgar R. Color and optical properties of 3D printing restorative polymer-based materials: A scoping review. *J Esthet Restor Dent* 2022;34:853–64. <https://doi.org/10.1111/jerd.12904>.
- [70] Bazos P, Magne P. Bio-Emulation: biomimetically emulating nature utilizing a histoanatomic approach; visual synthesis. *Int J Esthet Dent* 2014;9:330–52.